

부록6. 서식II-01-06, 온도기록지(IP 보관)

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2022.7
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2021.8.10		
	Certificate No.	SP2108-720R-06	Temperature Range	16~22℃(19±3℃)

Date	Time	Temperature(℃)			Verified by	Comment
		Min	Max	Current		
2022.07.01	P:30			19		
2022.07.02						
2022.07.03						
2022.07.04	P:30			19		
2022.07.05	P:30			19		
2022.07.06	P:30			19		
2022.07.07	P:40			19		
2022.07.08	P:30			19		
2022.07.09						
2022.07.10						
2022.07.11	P:30			19		
2022.07.12	P:30			19		
2022.07.13	P:30			19		
2022.07.14	P:30			19		
2022.07.15	P:30			19		
2022.07.16						
2022.07.17						
2022.07.18	P:30			19		
2022.07.19	P:40			19		
2022.07.20	P:30			19		
2022.07.21	P:45			19		
2022.07.22	P:30			19		
2022.07.23						
2022.07.24						
2022.07.25	P:30			18		
2022.07.26	P:30			19		
2022.07.27	P:20			19		
2022.07.28	P:30			19		
2022.07.29	P:30			19		
2022.07.30						
2022.07.31						


date of copying

sign

부록7. 서식II-01-07, 온도기록지(IP 보관)-자동온도 기록용지 부착형

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2022.6.30~2022.7.29
	Model Name	MPR-720R	Investigational Product	보관조건 15~25°C 25°C 1~25°C
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2021.8.10	Temperature Range	16~22°C(19±3°C)
	Certificate No.	SP2108-720R-06		

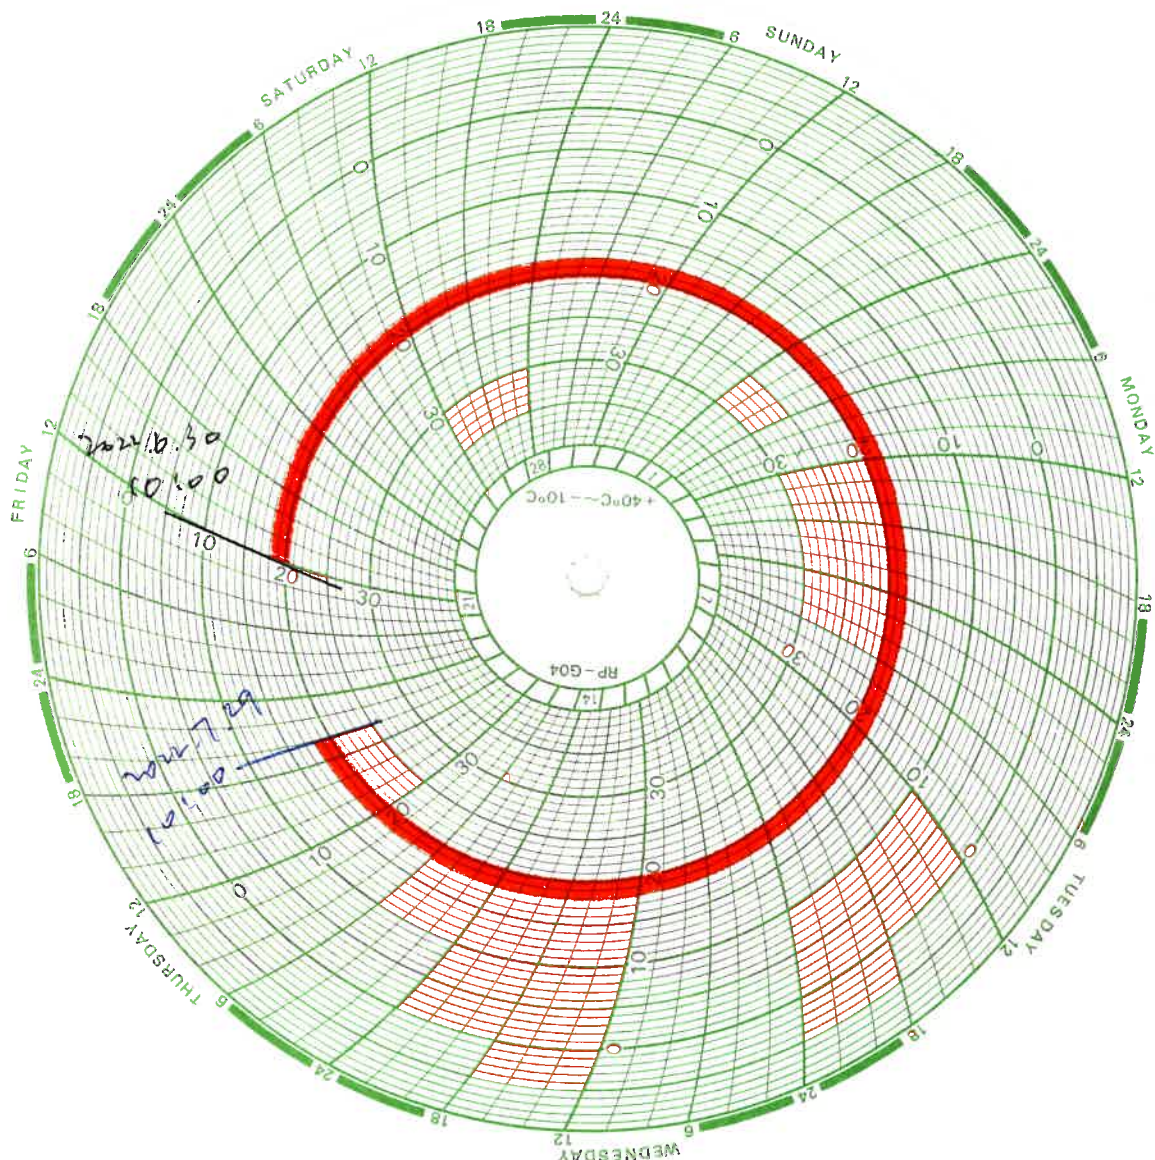

date of copying

sign