

부록6. 서식II-01-06, 온도기록지(IP 보관)

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2022.12
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5	Temperature Range	16~22℃(19±3℃)
	Certificate No.	SP2208-720R-07		

Date	Time	Temperature(℃)			Verified by	Comment
		Min	Max	Current		
2022.12.01	P:40			19		
2022.12.02	P:35			19		
2022.12.03						
2022.12.04						
2022.12.05	P:30			19		
2022.12.06	P:30			19		
2022.12.07	P:30			19		
2022.12.08	P:30			19		
2022.12.09	P:30			19		
2022.12.10						
2022.12.11						
2022.12.12	P:30			19		
2022.12.13	P:30			19		
2022.12.14	P:30			19		ATB IP 06d
2022.12.15	P:30			19		
2022.12.16	10:50			19		
2022.12.17						
2022.12.18						
2022.12.19	P:40			19		
2022.12.20	P:20			19		
2022.12.21	P:30			19		
2022.12.22	P:30			19		
2022.12.23	P:35			19		
2022.12.24						
2022.12.25						
2022.12.26	P:30			19		
2022.12.27	P:30			19		
2022.12.28	P:30			19		
2022.12.29	P:30			19		
2022.12.30	P:30			19		
2022.12.31						


date of copying

sign

부록7. 서식II-01-07, 온도기록지(IP 보관)-자동온도 기록용지 부착형

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2022.11.29~2022.12.10
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5		
	Certificate No.	SP2208-720R-07	Temperature Range	16~22℃(19±3℃)

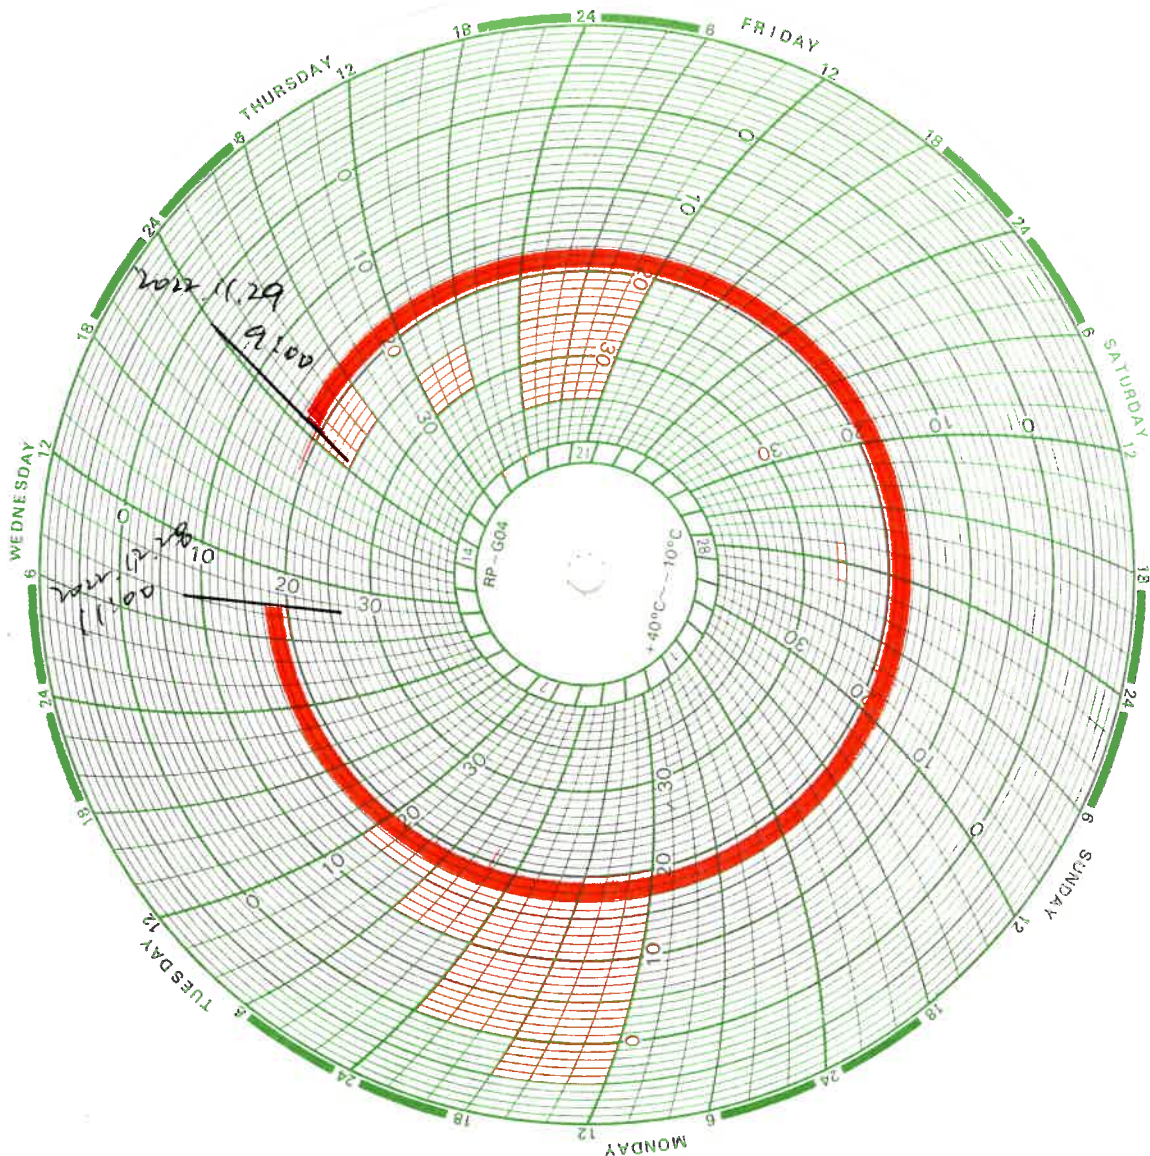

date of copying

sign