

부록6. 서식II-01-06, 온도기록지(IP 보관)

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2023.2
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5		
	Certificate No.	SP2208-720R-07	Temperature Range	16~22℃(19±3℃)

Date	Time	Temperature(℃)			Verified by	Comment
		Min	Max	Current		
2023.02.01	P:30			19	anf	
2023.02.02	P:30			18	anf	
2023.02.03	P:30			18	anf	
2023.02.04						
2023.02.05						
2023.02.06	P:30			19	anf	
2023.02.07	P:30			18	anf	
2023.02.08	P:40			18	anf	
2023.02.09	P:30			18	anf	
2023.02.10	P:30			18	anf	
2023.02.11						
2023.02.12						
2023.02.13	P:30			18	anf	
2023.02.14	P:30			18	anf	
2023.02.15	P:30			18	anf	
2023.02.16	P:30			18	anf	
2023.02.17	P:30			19	anf	
2023.02.18						
2023.02.19						
2023.02.20	P:30			19	anf	
2023.02.21	P:30			18	anf	
2023.02.22	P:30			18	anf	
2023.02.23	P:30			19	anf	
2023.02.24	P:30			19	anf	
2023.02.25						
2023.02.26						
2023.02.27	P:50			19	anf	HD-AI IP 보관
2023.02.28	P:30			18	anf	


date of copying

sign

부록7. 서식II-01-07, 온도기록지(IP 보관)-자동온도 기록용지 부착형

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2023.1.27~2023.2.16
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5		
	Certificate No.	SP2208-720R-07	Temperature Range	16~22℃(19±3℃)

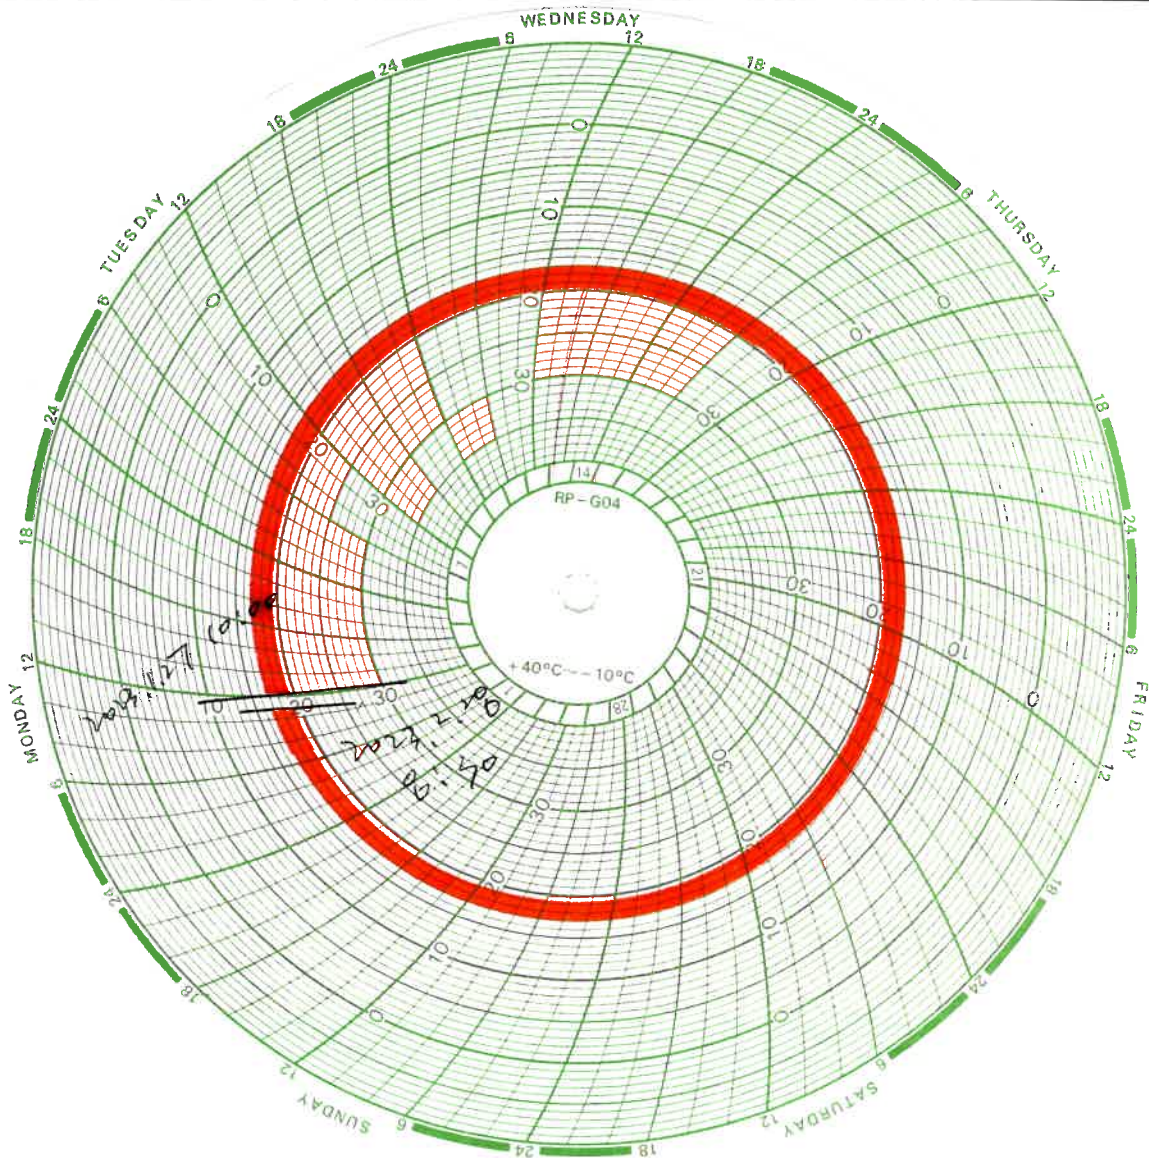

date of copying

sign