

부록6. 서식II-01-06, 온도기록지(IP 보관)

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2023.4
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5		
	Certificate No.	SP2208-720R-07	Temperature Range	16~22℃(19±3℃)

Date	Time	Temperature(℃)			Verified by	Comment
		Min	Max	Current		
2023.04.01						
2023.04.02						
2023.04.03	P:30			19		
2023.04.04	P:30			19		
2023.04.05	P:30			19		
2023.04.06	P:30			19		
2023.04.07	P:30			19		
2023.04.08						
2023.04.09						
2023.04.10	P:30			19		
2023.04.11	P:30			19		
2023.04.12	P:30			19		
2023.04.13	P:30			19		
2023.04.14	P:30			19		
2023.04.15						
2023.04.16						
2023.04.17	P:30			19		
2023.04.18	P:30			19		
2023.04.19	P:30			19		
2023.04.20	P:40			19		
2023.04.21	P:30			19		
2023.04.22						
2023.04.23						
2023.04.24	P:30			19		
2023.04.25	P:30			19		
2023.04.26	P:30			19		
2023.04.27	P:30			19		
2023.04.28	P:30			19		
2023.04.29						
2023.04.30						


date of copying

sign

부록7. 서식II-01-07, 온도기록지(IP 보관)-자동온도 기록용지 부착형

IP STORAGE TEMPERATURE LOG

Storage Subject	Description	전기냉장냉동기	Storage Space	항온고1
	Manufacturer	SANYO	Storage Period	2023.3.31~2023.4.28
	Model Name	MPR-720R	Investigational Product	보관조건 15~25℃ 25℃ 1~25℃
	Serial Number	07120004		
Calibration Subject	Description			
	Manufacturer			
	Model Name			
	Serial Number			
	Date of Calibration	2022.8.5		
	Certificate No.	SP2208-720R-07	Temperature Range	16~22℃(19±3℃)

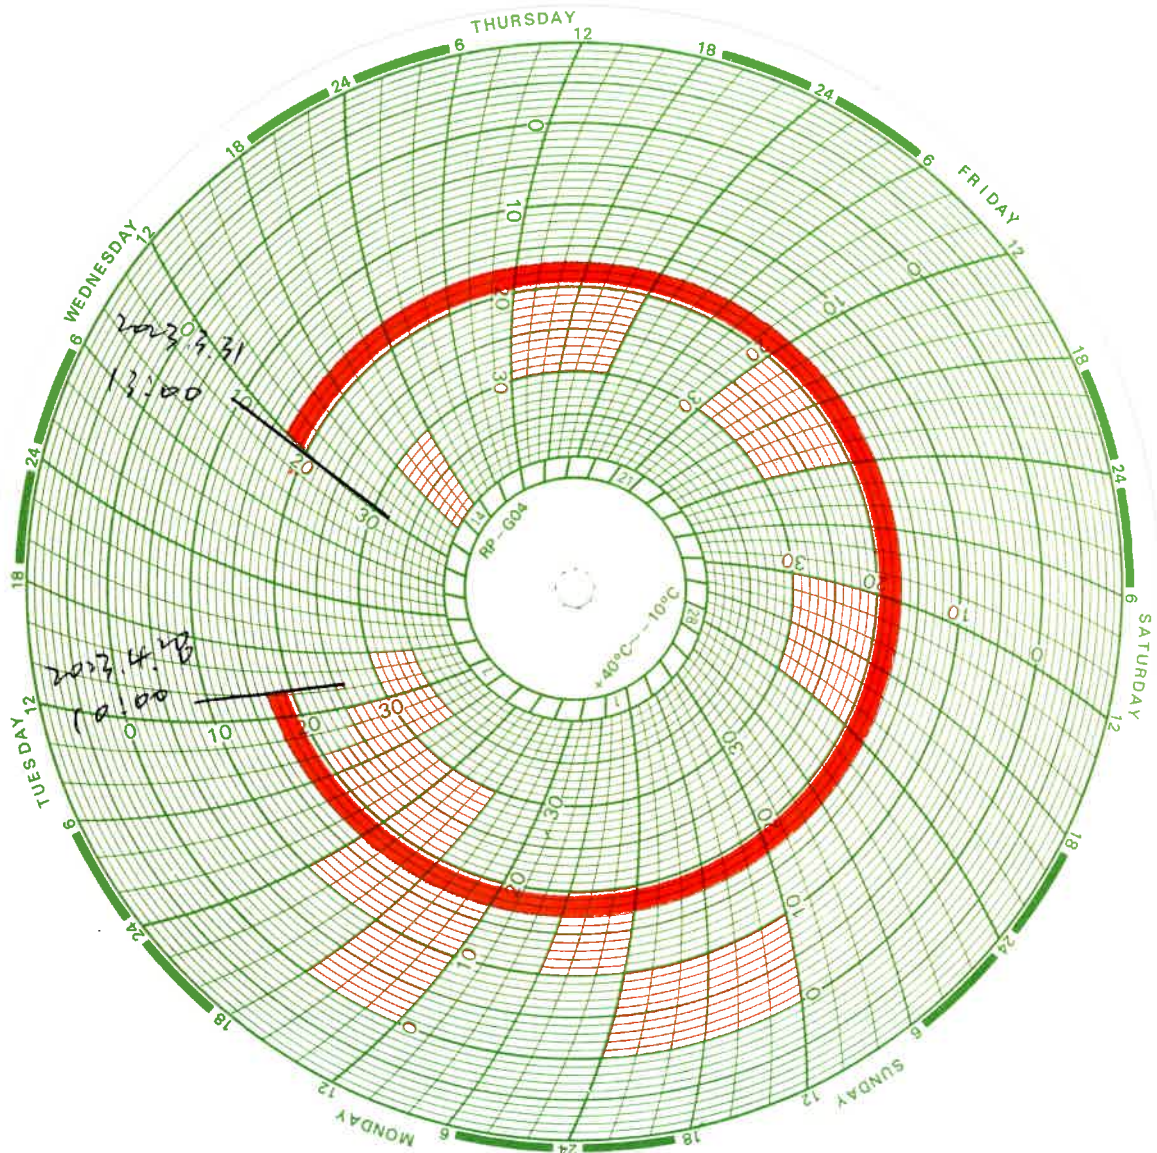

date of copying

sign